


Independently designed, relentlessly validated,
and meticulously engineered



HanSel MS

iQuad 2300 Series ICP-MS

A fusion of extraordinary sensitivity,
stability, and productivity

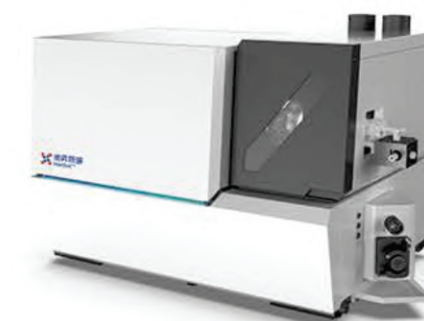

Reimagine elemental analysis with **Hansel ICP-MS**



Ruko Arya Kemuning Blok A No.4
Sukamaju, Kec. Cilodong, Kota Depok, Jawa Barat 16415

(021) 38741115

admin@adhyawaris.co.id

adhyawaris.co.id


PT. Adhya Waris Saintifik

@adhyascientific / @adhyawaris

iQuad 2300 Series

ICP-MS

A fusion of extraordinary sensitivity, stability, and productivity

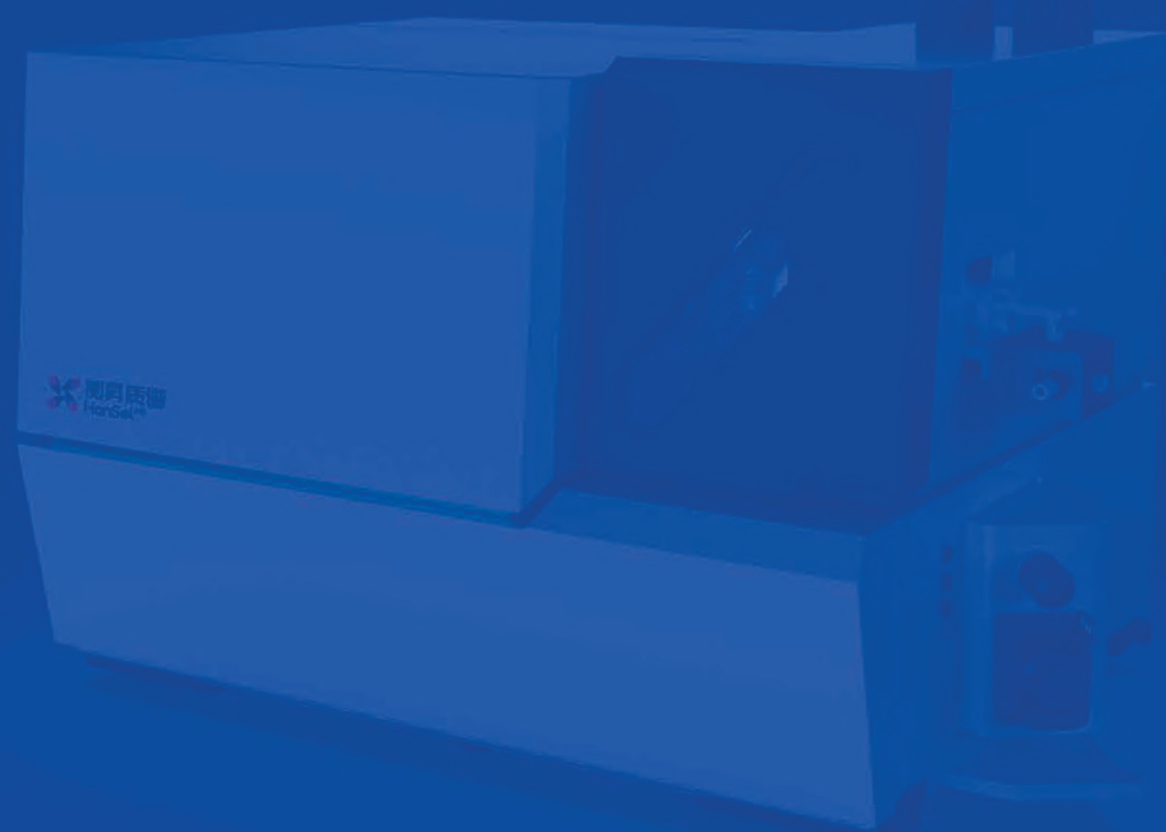


Independently designed, relentlessly validated, and meticulously engineered



Material

04

- Geological / Mineral / Metal material / New material
- Electronics / general consumer products
- Semi-conductor / photovoltaics / battery materials

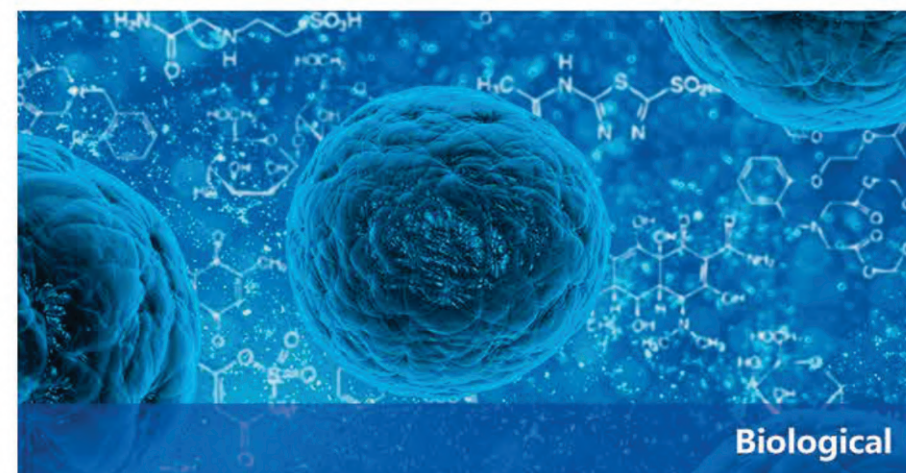

Biological

05

- Research in proteins, nucleic acids, and (single) cells
- Isotope-specific radiolabelling in immunology
- Nano-particle analysis



Energy & Chemical

06

- Petrochemical and generic chemical production
- Alternative energy research and development
- Specialized chemical material

Focused Application Fields

01

- Food safety regulatory development and enforcement
- Nutritional research in food
- Metal toxicity research in food



Food & Agriculture

02

- Environmental regulatory development and enforcement
- Heavy metal toxicity research in Water, soil, and air
- Metal toxicity research in solid waste
- Environmental emission monitoring



Environmental

03

- Help pharma industry normalize practices adhering to USP/EP/CP requirements
- Heavy metal toxicity in TCMs
- Metal toxicity research in clinical, gene-focused, and other life science applications



Pharma

CONTENTS

iQuad 2300 Series ICP-MS

Product Brochure

Product Overview

02

A Performance Beyond Your Expectation

04

Unrivalled sample throughput | Outstanding system stability | Superb data accuracy

iQuad 2300 Series: a Schematic View

08

Intelligent iTrace Software

10

Powerful data management system and much more

Focused Application Fields

12

Food / Agriculture | Environmental | Pharma | Material | Biological | Energy / Chemical

Product Overview

Hansel ICP-MS A Ten-Year Journey

iQuad 2300 Series ICP-MS



2014

- Founding of Hansel

2016

- Kick-off of ICP-MS project

2018



- 1st gen. ICP-MS prototype

2021



- 2nd gen. ICP-MS prototype and validation

2022



- Production of iQuad series ICP-MS began
- Launch of iQuad 2300 ICP-MS modernization project

2023



- Commercial launch of iQuad 2300 series

...

Intuitive and powerful software operation — extremely friendly for beginners and experts alike

- Simplified method development dashboard
- Simultaneous sample analysis and data processing capability
- Advanced data acquisition in chromatographic, nano-particle, and single-cell applications

Alternative APP-based operation — an ICP-MS at your fingertip

- Delayed system start, remote system start, and automatic plasma off
- Unattended sample analysis achieved via intelligent cellphone app



Uncompromising regulatory compliance to protect data integrity

- FDA 21CFR Part 11 compliant
- User access control, data validation and security, e-signature and audit trail
- Open to customize and implement special regulatory requirements

Intelligent iTrace Software


iTrace

Expert software designed for multi-element ICP-MS analysis



iTrace – convenience, accessibility, and advanced applications

- One button “Get Start”
- System auto-tune
- Comprehensive quality control
- Speciation, nano-particle, single-cell analysis
- Laser ablation analysis

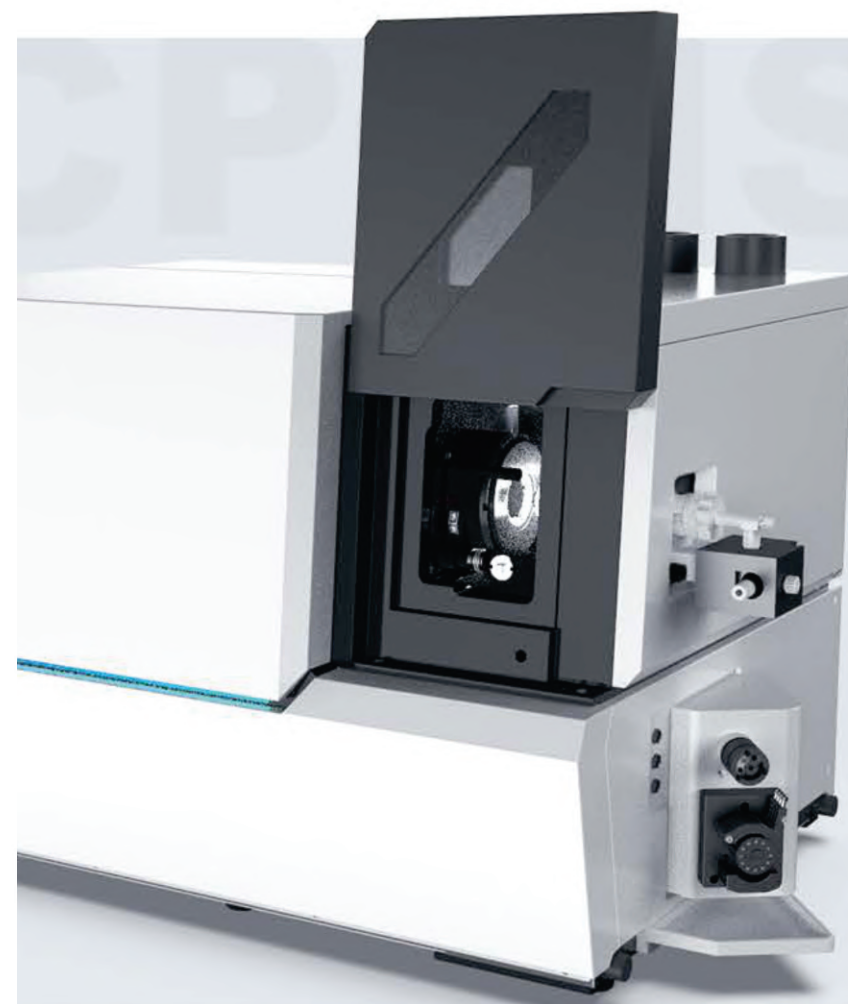

After 5 years of unrelenting R&D efforts, the robust 2nd generation iQuad ICP-MS was commercially launched in 2022, featuring technological innovations and breakthroughs in core functional modules such as digitally synthesized RF generator and humidity / temperature indiscriminate quadrupole mass analyzer.

Hansel's endeavor to further improve the performance and user friendliness of iQuad ICP-MS did not stop there. Merely one year later, the release of an extensively modernized iQuad 2300 in July 2023, incorporating an upgraded 7-port rapid sample introduction system, enhanced hexapole collision/reaction cell with axial acceleration, one-button system initiation and app-based remote instrument control, substantially elevated its sample throughput capability and overall competitiveness in the single-quad ICP-MS category.

Performance Highlights

-  Mature interference removal
-  Superb handling of complex matrices
-  Rapid sample analysis and data acquisition




A Performance Beyond Your Expectation

01 Unrivalled sample throughput

- 7-port high speed sample introduction system—reduce per sample analysis time up to 50%




Equipped with a high-speed uptake pump, the 7-port high speed sample introduction system allows sample loading and rinsing to execute simultaneously. This discrete sampling technology achieves drastically improved sample throughput and substantially reduced argon consumption for the customer.

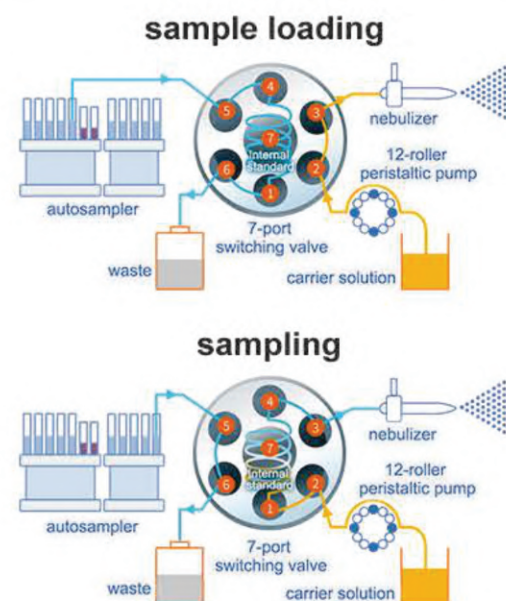

The 7-port high speed sample introduction system effectively diminishes the 'dead time' in conventional ICP-MS analysis while greatly improving the efficiency up to 50%.

Sample throughput
50%+

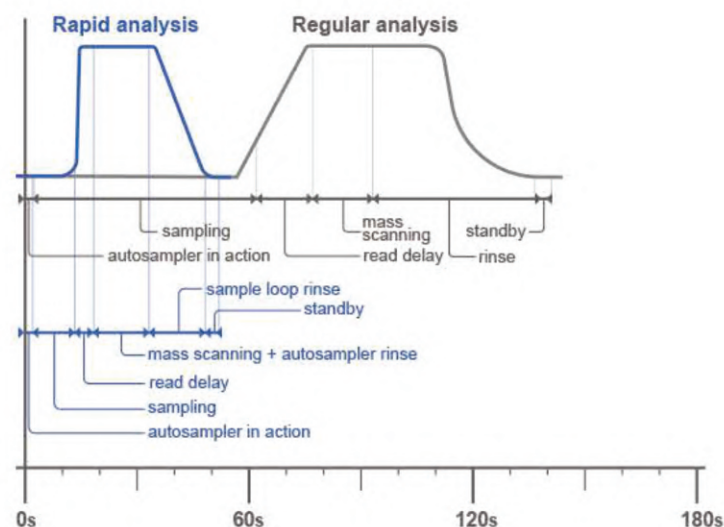

High-precision collision/reaction cell

- High transmission hexapole
- Mature KED (Kinetic Energy Discrimination) and SER (Selected Exothermic Reaction) dual mode interference removal

Robust Plasma Interface

- Water cooled sampling and skimmer cones, with nickel and platinum options
- Robust design ensures steady high matrix tolerance and low contamination in the vacuum



Formidable plasma RF generator

- 27.12 MHz with variable-frequency impedance matching
- Matching box free
- Virtual Grading designing, without Shield Torch
- Digitally driven and maintenance free
- Convenient switching between cold/hot plasma
- Plasma TV

Reliable and customizable sample introduction system

- Standard concentric nebulizer and cyclonic spray chamber (Scott Double-pass optional)
- Compatible with all mainstream nebulizers (high purity quartz, PTFE, PFA)
- 4-channel, 12-roller peristaltic pump with speed control
- 7-port switching valve available for high-speed discrete sampling
- Automatic X-Y-Z alignment and sampling depth optimization
- Standard Peltier cooled spray chamber optimizes signal drift

iQuad 2300 Series: a Schematic View

iQuad 2300 Series ICP-MS


An ICP-MS of exceptional matrix handling capability

High-performing quadrupole mass analyzer driven by digitally synthesized RF generator

- Matching box and air capacitor free
- Delivers superior peak separation and abundance sensitivity
- No custom quadrupole setting required

High-sensitivity electron multiplier detector

- Classic analog/pulse dual mode
- Linear dynamic range $>10^{11}$ (with electronic dilution)
- 10 μ s minimum integration time

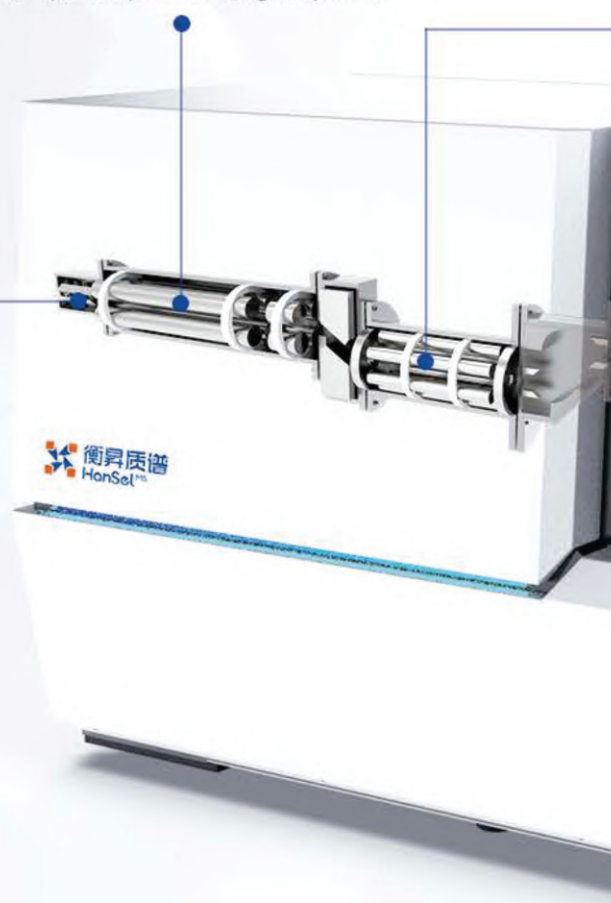

Beyond the conventional ICP-MS applications

- Compatible with various autosamplers and auto-dilution devices (CETEC, ESI)
- Direct solid analysis with laser ablation
- LC, GC, IC hyphenation for speciation analysis
- Nano-particle and single-cell analysis

- **Intelligent electronic dilution technology**—Simultaneous determination of isotopes from ultratrace level to 1000s of ppm.

The per-isotope electronic dilution can effectively extend the linear dynamic range up to 11 orders of magnitude and enable the system to analyze extremely low and high concentration isotopes in the same sample simultaneously, thus greatly improve the analytical efficiency for customers tasked to analyze multi-elements in a large number of samples on a daily basis.

Case study: electronic dilution used for rich elements in food applications


	Identifier	Δ	Dwell time (s)	Channels	Spacing (u)	Measurement mode	ΔH	Resolution
▶	23Na (KED)		0.05	3	0.05	KED	0.17	Normal
	27Al (KED)		0.05	3	0.05	KED	0.04	Normal
	52Cr (KED)		0.05	3	0.05	KED	0	Normal
	60Ni (KED)		0.05	3	0.05	KED	0	Normal
	75As (KED)		0.05	3	0.05	KED	0	Normal
	114Cd (KED)		0.05	3	0.05	KED	0	Normal
	208Pb (KED)		0.05	3	0.05	KED	0.04	Normal

Analyte/Isotope	Concentration	Unit	Pre-dilution	ΔH	Post-dilution	Dilution factor
Na 23	100	mg/L	212,235,821	0.17	934,605	227.09
Al 27	5	mg/L	3,713,367	0.04	679,693	5.46
Cr 52	50	μ g/L	890,056	0	916,519	0.97
Ni 60	50	μ g/L	367,205	0	375,734	0.98
As 75	50	μ g/L	63,288	0	66,699	0.95
Cd 114	50	μ g/L	431,550	0	441,591	0.98
Pb 208	50	μ g/L	3,615,170	0.04	740,711	4.88

- **Intelligent one-button system start**—accessibility enhanced by remote control and system monitoring

Get Start Analytical results one button away


- ✓ Water chiller on
- ✓ Plasma ignition
- ✓ Plasma stabilization
- ✓ Auto-tune
- ✓ Performance test
- ✓ Sample analysis
- ✓ QC and data validation
- ✓ Generate QC report
- ✓ Plasma off, system standby
- ✓ Delayed system kick-off
- ✓ Remote system kick-off

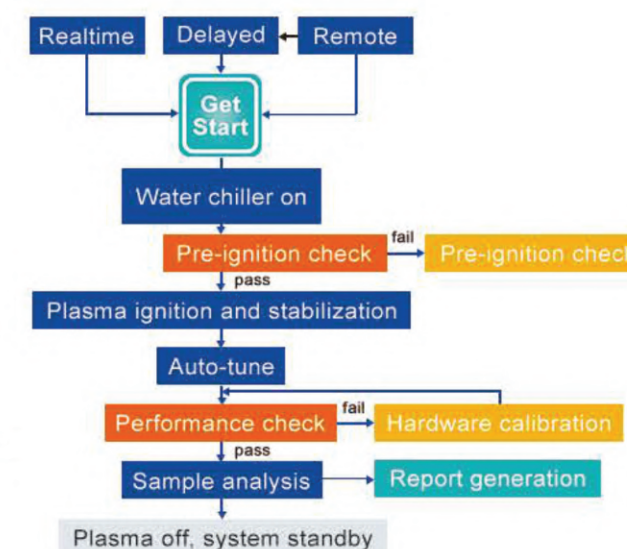

02 Outstanding system stability

No.	7Li	59Co	115In	238U	137Ba++ / 137Ba	140Ce.16O / 140Ce
1	35169.11	63695.03	143033.64	193412.83	0.013	0.019
2	34828.15	61363.40	140085.49	197668.85	0.013	0.019
3	35581.29	63435.63	140800.47	188159.45	0.014	0.018
4	35298.21	63157.60	142939.57	200100.06	0.013	0.018
5	34402.31	59915.74	136914.74	192500.20	0.012	0.019
6	35743.75	64604.65	145690.10	195153.79	0.013	0.019
7	35994.83	63345.51	143522.20	201375.94	0.013	0.020
8	35409.80	62684.89	139771.80	187928.48	0.014	0.018
9	35520.12	62701.97	140283.71	191576.21	0.012	0.018
10	34350.19	60182.03	133546.26	184133.56	0.014	0.017
11	35938.62	64111.11	141044.28	194223.83	0.014	0.020
12	35849.41	64398.22	142915.65	195977.76	0.013	0.020
13	35240.00	61654.73	138869.07	194766.82	0.012	0.018
14	36254.23	63555.29	141887.23	195740.75	0.014	0.019
15	36056.99	63862.82	143596.09	190340.55	0.014	0.018
16	36280.63	63378.78	141276.64	198492.23	0.014	0.018
17	35871.53	63768.74	142059.42	197573.87	0.013	0.018
18	36614.62	65547.87	143365.83	187154.46	0.013	0.017
19	36343.15	64296.39	140842.78	189302.88	0.014	0.017
20	36018.88	63176.04	139355.79	189252.79	0.014	0.017
21	36330.12	64082.62	141106.67	181462.68	0.014	0.017
22	36738.64	65497.30	142501.75	187722.62	0.014	0.018
23	36786.43	64875.01	144125.87	193187.47	0.013	0.018
24	36138.24	63243.67	140812.15	192415.04	0.014	0.019
AVG	35781.64	63355.63	141264.47	192484.30	1.34%	1.83%
SD	661.39	1424.18	2528.61	4992.20		
RSD	1.85%	2.25%	1.79%	2.59%		

- Extraordinary long-term stability – 4 hour signal drift RSD< 3%

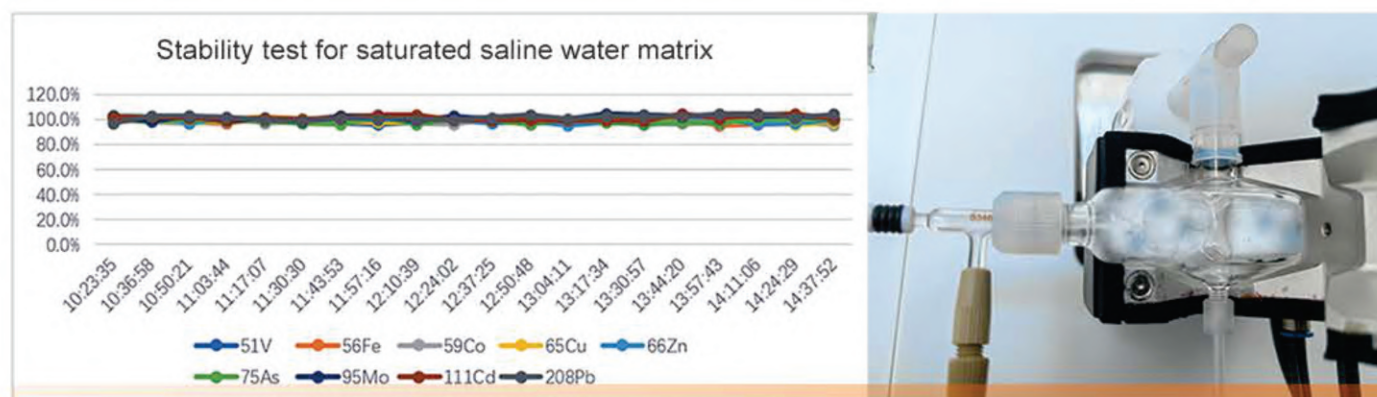


- Online aerosol dilution – tackles the most complex and challenging sample matrices



- One of the longest quadrupole mass analyzer in the industry – source of highly reproducible data

03 Superb data accuracy

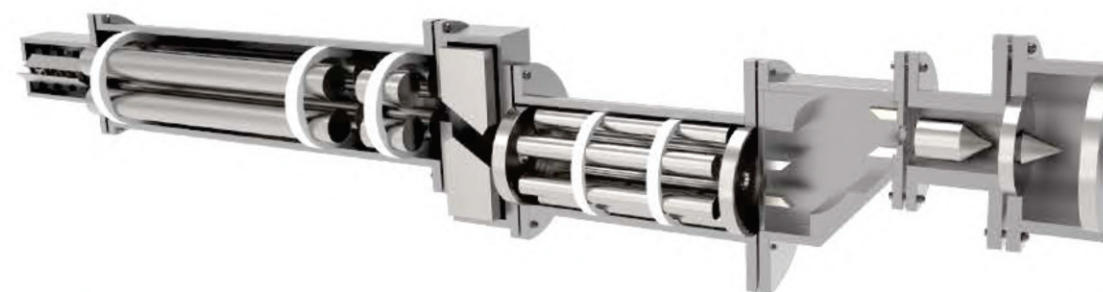

- Streamlined hexapole collision/reaction cell permits efficient removal of polyatomic interferences.
- Proprietary axial acceleration technology drastically improves the ion transmission efficiency and overall sensitivity.
- High performing ion optics and the dual off-axis ion pathway work to effectively eliminate neutral particles in the post plasma ion beam, substantially reducing the background of the analysis.

Analytical results of GBW E 080684, a Rice Powder CRM

Element	Concentration	Spike recovery	Measured value	Certified value
Na	ppm	106.2%	8.79	8±1
Mg	ppm	104.6%	261.66	252±23
K	ppm	93.1%	997.24	1060±70
Ca	ppm	106.8%	66	67.3±8.4
Mn	ppm	103.9%	11.772	12.4±0.7
Fe	ppm	95.9%	4.49	4.7±0.6
Cu	ppm	101.3%	1.77	1.97±0.23
Zn	ppm	94.0%	11.7	13±1.3
As	ppm	101.8%	0.11	0.11±0.02
Se	ppm	94.4%	53.51	45±15
Cd	ppm	99.5%	0.0075	0.009±0.004
Pb	ppm	98.9%	0.015	0.024±0.01